bürkert
FLUID CONTROL SYSTEMS









Chlorine (Cl_2) or chlorine dioxide (ClO_2) Sensor Cube

- Fully compatible with büS systems and a wide range of further analysis sensor cubes
- Optional pH compensated chlorine measurement
- Modular sensor cube for hot swap (exchange during operation)
- Minimal sample water flow needed
- MEMS technology sensor

Product variants described in the data sheet may differ from the product presentation and description.

Can be combined with



Type 8905 ▸
Online Analysis System



Type 8920 ▸
Bürkert Communicator

Type description

The device is selectable to measure chlorine or chlorine dioxide in water. It is used within the Online Analysis System Type 8905 by being plugged into a spare fluidic backplane slot.

The sensor cube contains a high precision membrane covered amperiometric sensor, based on Bürkert microelectromechanical systems technology (MEMS). The measurement signal shows the Cl_2 or ClO_2 content within the sample water. The chlorine measurement reflects either the available chlorine HOCl or, if coupled with a MS01 pH sensor cube for pH compensation, the free chlorine.

The electrical and fluidic connections are made via the connection panel of the system. The sensor cube is communicating with the system via büS, allowing fully automatic login to the online analysis system. If the sensor is plugged into the system, it automatically logs on to the büS and can be parameterised according to customer requirements.

powered by EDIP büS

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

© Christian Bürkert GmbH & Co. KG, Subject to alteration

Visit product website ▸

Table of contents

1. General technical data 3

2. Materials 4

2.1. Chemical Resistance Chart – Bürkert resistApp....4

3. Dimensions 5

4. Product installation 5

4.1. Installation notes....5

5. Product design and assembly 6

5.1. Product features....6

6. Ordering information 6

6.1. Bürkert eShop – Easy ordering and quick delivery....6
6.2. Bürkert product filter....6
6.3. Ordering chart....7
6.4. Ordering chart accessories....7

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

1. General technical data


Product properties	
Material	
Please make sure the device materials are compatible with the fluid you are using. Detailed information can be found in chapter "2.1. Chemical Resistance Chart – Bürkert resistApp" on page 4.	
Housing	PPE+PS
Lever	Zamak, painted
Seals	EPDM
Dimensions	Detailed information can be found in chapter "3. Dimensions" on page 5.
Chlorine/chlorine dioxide sensor	Membrane covered PT-cell, amperiometric 3 electrodes measurement, without electrolyte
Temperature sensor	Pt1000 Class B, no contact with the water sample
Compatibility	With Online Analysis System Type 8905 (the electrical and fluidic contact is made via backplane system.) Detailed information can be found in the data sheet of the online analysis system, see **data sheet Type 8905** ▶ for more information.
Measuring range	
Chlorine measurement (Cl_2)	0.01…5 ppm
Chlorine measurement (ClO_2)	0.005…5 ppm
Maintenance	12 months nominal, depending on the water quality
Performance data	
Chlorine measurement (Cl_2)	
Sensitivity	-11 nA/ppm (at pH 5), -8 nA/ppm (at pH 7)
pH compensation	Yes, with MS01 sensor cube Detailed information can be found in the data sheet of the pH sensor cube, see **data sheet Type MS01** ▶ for more information
Measuring range resolution	0.01 ppm
Measurement deviation	±0.03 ppm or ±5 % of the measured value
Linearity	±0.02 ppm of the measured value
Repeatability	±0.02 ppm of the measured value
Response time (t_{90})	<30 s
Chlorine measurement (ClO_2)	
Sensitivity	-4 nA/ppm
pH compensation	No
Measuring range resolution	0.001 ppm
Measurement deviation	±0.005 ppm or ±3 % of the measured value (the greater value applies)
Linearity	±0.01 ppm or ±3 % of the measured value (the greater value applies)
Repeatability	±0.01 ppm or ±3 % of the measured value (the greater value applies)
Response time (t_{90})	<30 s
Temperature measurement	0…+50 °C (+32…+122 °F)
Electrical data	
Operating voltage	24 V DC through the backplane of the system Type 8905 via büS
Power consumption	0.8 VA
Media data	
Fluid	Water without particles: drinking water, industrial water
pH range	pH 4…pH 9
Conductivity	>50 µs/cm
Sample water	
Temperature	+3…+40 °C (+37…+104 °F)
Pressure	PN3
Flow rate	>6 l/h
Process/Port connection & communication	
Process connection	Via pinch valve in the fluidic backplane of the Type 8905 Detailed information can be found in the data sheet of t the Online Analysis System, see **data sheet Type 8905** ▶ for more information.

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

Electrical connection	Spring contacts in the fluidic backplane of the Type 8905, which is connected to a büS System Detailed information can be found in the data sheet of t the Online Analysis System, see **data sheet Type 8905** ▶ for more information.
Data transfer	
Internal communication	Through büS (Bürkert bus, CANopen protocol)
External communication by status LED	According to NAMUR NE 107
Approvals and Certificates	
Standards	
Protection class according to IEC/ EN 60529	• IP65, when plugged in the fluidic backplane • IP20, as standalone product
Directives	
CE directives	The applied standards, which verify conformity with the EU Directives, can be found on the EU Type Examination Certificate and/or the EU Declaration of conformity (if applicable).
Environment and installation	
Ambient temperature	
Operating	+3…+40 °C (+37…+104 °F)
Storage and transport	For empty/purged sensor cube: -10…+60 °C (+14…+140 °F)
Relative air humidity	≤90 %, without condensation
Height above sea level	Max. 2000 m
Operating condition	Continuous
Equipment mobility	Fixed
Application range	Indoor and outdoor (Protect the device against electromagnetic interference, ultraviolet rays and, when installed outdoors, against the effects of climatic conditions)
Installation category	Category I according to UL/EN 61010-1
Pollution degree	Degree 2 according to UL/EN 61010-1

2. Materials

2.1. Chemical Resistance Chart – Bürkert resistApp

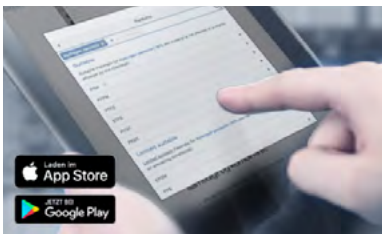

Bürkert resistApp – Chemical Resistance Chart


You want to ensure the reliability and durability of the materials in your individual application case? Verify your combination of media and materials on our website or in our resistApp.

Start Chemical Resistance Check

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

3. Dimensions

Note:
Dimensions in mm

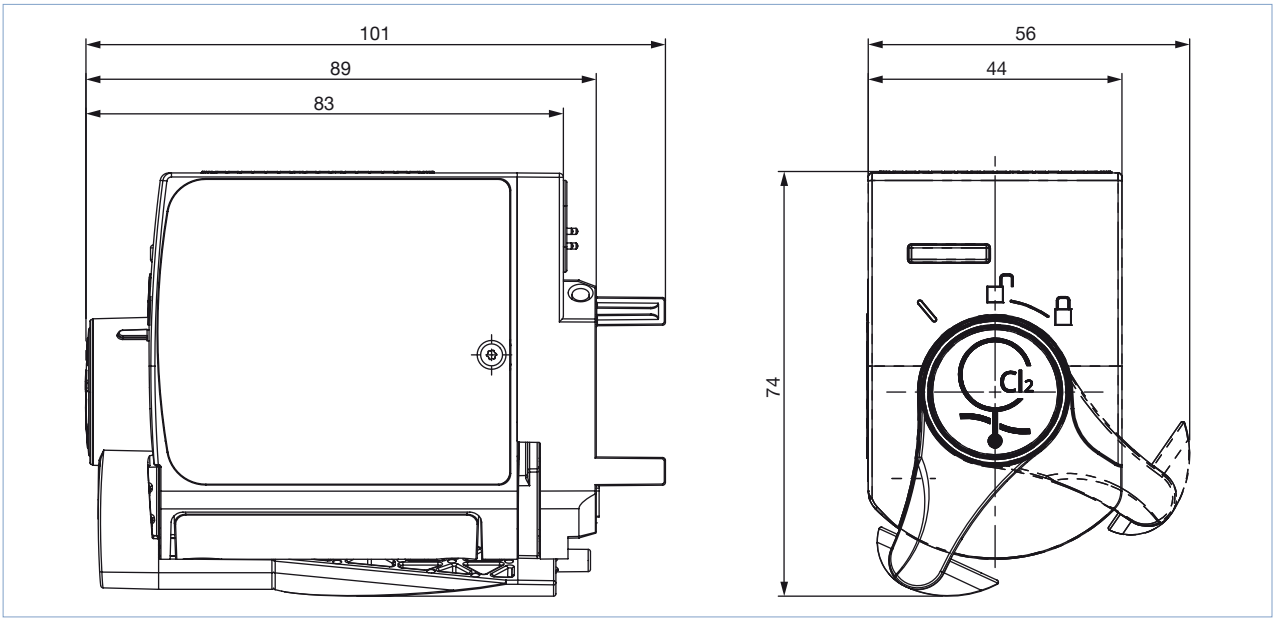


4. Product installation

4.1. Installation notes

Note:

- The sensor cube is designed for use with the online analysis system, Type 8905. The sensor cube is simply plugged into the backplane in Type 8905.
- It is also possible to mount the backplane individually on a DIN rail.


See **data sheet Type 8905** ▸ Online Analysis System for more information.

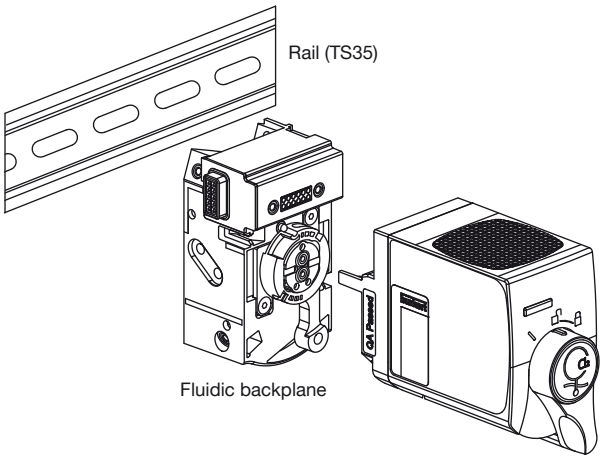Installation examples	
Product mounted in a housing for the Online analysis system Type 8905. • Chlorine or chlorine dioxide sensor cube Type MS02 • Housing Type 8905 with display Type ME21 and controller Type ME25 	**Product without housing mounted of the backplane on standard rail (TS35).** 

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

5. Product design and assembly

5.1. Product features

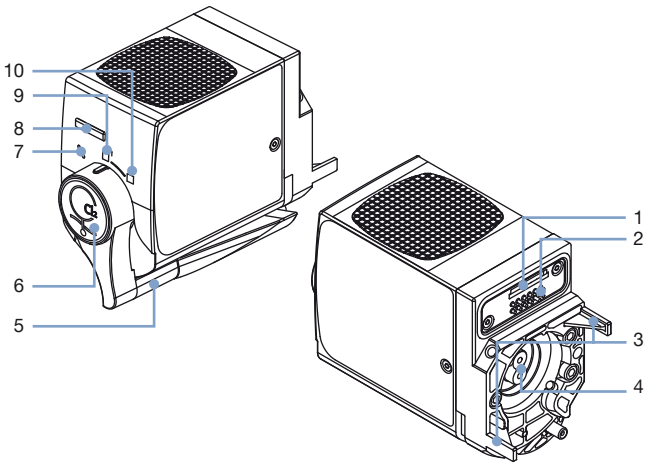

Product without housing

No.	Element
1	Slot micro-SIM card (for configuration data)
2	Electrical interface
3	Guide pins
4	Fluid connections
5	Lever to: • lock / unlock the product • carry out maintenance operations
6	Push button for unlocking
7	Maintenance position
8	Sensor cube Status LED
9	Unlocked position
10	Locked position

6. Ordering information

6.1. Bürkert eShop – Easy ordering and quick delivery



Bürkert eShop – Easy ordering and fast delivery

You want to find your desired Bürkert product or spare part quickly and order directly? Our online shop is available for you 24/7. Sign up and enjoy all the benefits.

Order online now

6.2. Bürkert product filter



Bürkert product filter – Get quickly to the right product

You want to select products comfortably based on your technical requirements? Use the Bürkert product filter and find suitable articles for your application quickly and easily.

Try out our product filter

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

6.3. Ordering chart

Note:
The chlorine/chlorine dioxide sensor cube must be operated within a system.

Please refer to the order information for Online Analysis System Type 8905, see **data sheet Type 8905** ▸ or contact your Bürkert representative.

Description	Article no.
Chlorine (Cl_2) sensor cube	567625
Chlorine dioxyde (ClO_2) sensor cube	567721

6.4. Ordering chart accessories

Description	Article no.
Photometer MD100, measuring range 0.01…6 ppm	566393
DPD-1 reagent (100 Tablets)	566394
Replacement part set: measurement cell	568040

DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

Bürkert – Close to You

For up-to-date addresses
please visit us at
www.burkert.com



DTS 1000220807 EN Version: K Status: RL (released | freigegeben | validé) printed: 12.01.2021

Credits, © and concept: Christian Bürkert GmbH & Co. KG | Photographs: Marc Eggimann Fotografie - 4051 Basel | Scanner GmbH - Werbeagentur Künzelsau - 74653 Künzelsau